

# 100 kSps, 16-bit, High-throughput $\Delta\Sigma$ ADC Evaluation Board

## Features

- ❑ Analog Input Channels to the CS5571 ADC
- ❑ Pre-configured to require a minimum number of external connections to your data acquisition system.
- ❑ All functionality accessible through the connector interface and board-level options.
- ❑ On-board 4.096 V Reference
- ❑ Pre-configured for Master mode SPI™ communication to a data capture system.

## General Description

The CDB5571 is a versatile tool designed for evaluating the functionality and performance of the CS5571 ADC (Analog-to-Digital Converter). The SPI serial port on the CDB5571 evaluation board is configured in Master mode and will start transmitting data after power-up upon reset. This evaluation board is designed to connect to your data capture system or will interface to the CapturePlus II data acquisition system available from Cirrus Logic.

The CS5571 delta-sigma ADC produces fully settled conversions to full specified accuracy at 100 kSps. This ability to produce fully settled conversions for every sample makes it suitable for converting multiplexed input signals. To help evaluate this feature, the CDB5571 includes two single-ended analog inputs multiplexed into the CS5571. The multiplexer can be switched at the CS5571 ADC sample speed and the ADC will produce fully settled conversion data for each input channel.

All evaluation board functionality for evaluating the CS5571 ADC is accessed through the connector interface and board-level options.


Schematics in PADS™ PowerLogic™ format are available for download at:

<http://www.cirrus.com/en/products/pro/detail/P1120.html>.

## ORDERING INFORMATION

CDB5571

Evaluation Board



---

## Contacting Cirrus Logic Support

For all product questions and inquiries contact a Cirrus Logic Sales Representative. To find the one nearest to you go to [www.cirrus.com](http://www.cirrus.com)

---

### IMPORTANT NOTICE

Cirrus Logic, Inc. and its subsidiaries ("Cirrus") believe that the information contained in this document is accurate and reliable. However, the information is subject to change without notice and is provided "AS IS" without warranty of any kind (express or implied). Customers are advised to obtain the latest version of relevant information to verify, before placing orders, that information being relied on is current and complete. All products are sold subject to the terms and conditions of sale supplied at the time of order acknowledgment, including those pertaining to warranty, indemnification, and limitation of liability. No responsibility is assumed by Cirrus for the use of this information, including use of this information as the basis for manufacture or sale of any items, or for infringement of patents or other rights of third parties. This document is the property of Cirrus and by furnishing this information, Cirrus grants no license, express or implied under any patents, mask work rights, copyrights, trademarks, trade secrets or other intellectual property rights. Cirrus owns the copyrights associated with the information contained herein and gives consent for copies to be made of the information only for use within your organization with respect to Cirrus integrated circuits or other products of Cirrus. This consent does not extend to other copying such as copying for general distribution, advertising or promotional purposes, or for creating any work for resale.

CERTAIN APPLICATIONS USING SEMICONDUCTOR PRODUCTS MAY INVOLVE POTENTIAL RISKS OF DEATH, PERSONAL INJURY, OR SEVERE PROPERTY OR ENVIRONMENTAL DAMAGE ("CRITICAL APPLICATIONS"). CIRRUS PRODUCTS ARE NOT DESIGNED, AUTHORIZED OR WARRANTED FOR USE IN PRODUCTS SURGICALLY IMPLANTED INTO THE BODY, AUTOMOTIVE SAFETY OR SECURITY DEVICES, LIFE SUPPORT PRODUCTS OR OTHER CRITICAL APPLICATIONS. INCLUSION OF CIRRUS PRODUCTS IN SUCH APPLICATIONS IS UNDERSTOOD TO BE FULLY AT THE CUSTOMER'S RISK AND CIRRUS DISCLAIMS AND MAKES NO WARRANTY, EXPRESS, STATUTORY OR IMPLIED, INCLUDING THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR PARTICULAR PURPOSE, WITH REGARD TO ANY CIRRUS PRODUCT THAT IS USED IN SUCH A MANNER. IF THE CUSTOMER OR CUSTOMER'S CUSTOMER USES OR PERMITS THE USE OF CIRRUS PRODUCTS IN CRITICAL APPLICATIONS, CUSTOMER AGREES, BY SUCH USE, TO FULLY INDEMNIFY CIRRUS, ITS OFFICERS, DIRECTORS, EMPLOYEES, DISTRIBUTORS AND OTHER AGENTS FROM ANY AND ALL LIABILITY, INCLUDING ATTORNEYS' FEES AND COSTS, THAT MAY RESULT FROM OR ARISE IN CONNECTION WITH THESE USES.

Cirrus Logic, Cirrus, and the Cirrus Logic logo designs are trademarks of Cirrus Logic, Inc. All other brand and product names in this document may be trademarks or service marks of their respective owners.

SPI is a trademark of Motorola, Inc.

PADS and PowerLogic are trademarks of Mentor Graphics.

**TABLE OF CONTENTS**

<b>1. INTRODUCTION</b> .....	<b>4</b>
1.1 Overview .....	5
<b>2. QUICK START</b> .....	<b>6</b>
<b>3. HARDWARE DESCRIPTION</b> .....	<b>7</b>
3.1 Absolute Maximum Ratings .....	7
3.2 Power Supply .....	7
3.3 Analog Section .....	7
3.3.1 Analog Input Buffers .....	7
3.3.2 Multiplexer .....	8
3.3.3 ADC Reset .....	8
3.3.4 Voltage Reference .....	8
3.3.5 ADC Reference Frequency .....	8
3.4 Digital Section .....	9
3.4.1 Hardware Configuration .....	9
3.4.2 SPI™ Serial Port Communications .....	9
<b>Appendix A. Maximizing the Performance of the CS5571</b> .....	<b>10</b>
A.1 PCB Layout Considerations .....	10
A.2 Hardware Considerations.....	10
<b>Appendix B. Bill Of Materials</b> .....	<b>11</b>
<b>Appendix C. Schematics</b> .....	<b>12</b>
<b>Appendix D. Layer Plots</b> .....	<b>17</b>
<b>REVISION HISTORY</b> .....	<b>26</b>

**LIST OF FIGURES**

Figure 1. CDB5571 Block Diagram .....	5
Figure 2. CDB5571 Board Layout.....	6
Figure 3. Schematic - Block Diagram.....	12
Figure 4. Schematic - Power Supplies.....	13
Figure 5. Schematic - Input Buffers and Multiplexer .....	14
Figure 6. Schematic - CS5571 .....	15
Figure 7. Schematic - Configuration & Misc.....	16
Figure 8. Top Silkscreen .....	17
Figure 9. Top Solder Mask.....	18
Figure 10. Top Routing .....	19
Figure 11. Ground Plane.....	20
Figure 12. Power Plane.....	21
Figure 13. Bottom Solder Mask.....	22
Figure 14. Bottom Silkscreen .....	23
Figure 15. Top Solder Paste Mask.....	24
Figure 16. Bottom Routing .....	25

**LIST OF TABLES**

Table 1. Power Supply Connections .....	7
Table 2. Analog Input Connections .....	7
Table 3. Analog Input Channel Selection .....	8
Table 4. Hardware Configuration Signals .....	9
Table 5. Serial Interface Connections .....	9

## 1. INTRODUCTION

The CDB5571 evaluation board is a platform for evaluating the CS5571 ADC performance. The evaluation board is designed to connect to the SPI serial port of a processor or data capture system or will interface directly to the CapturePlus II data acquisition system available from Cirrus Logic. The CapturePlus II data acquisition system is a powerful integrated hardware/software tool designed to fully exercise the CDB5571 and other Cirrus Logic evaluation boards.

The CDB5571 evaluation board is designed to simplify the hardware setup required to evaluate the CS5571. Interfacing the CDB5571 evaluation board to a user-supplied data capture system can be as simple as connecting the SPI port and using the CDB5571 default hardware configuration. In this configuration simply press the Reset switch on the CDB5571 and it will automatically begin transmitting data to the data capture system.

All evaluation board functionality for evaluating the CS5571 ADC is accessed through the connector interface and board-level options.

The CS5571 delta-sigma ADC produces fully settled conversions to full specified accuracy at 100 kSps. The ability to produce fully settled conversions for every sample makes it suitable for converting multiplexed input signals. To help evaluate this feature, the CDB5571 includes two single-ended analog inputs multiplexed into the CS5571. The multiplexer can be switched at the CS5571 ADC sample speed and the ADC will produce fully settled conversion data for each input channel.

For detailed information on the CS5571 ADC, please reference data sheet DS768 at [www.cirrus.com](http://www.cirrus.com).

## 1.1 Overview

The CDB5571 evaluation board has both analog and digital circuit sections. The analog section consists of the CS5571 ADC, two analog input signal buffers, controlled through a multiplexer, that condition the signals into the ADC, and a precision 4.096 V reference. The digital section consists of board operation configuration control signals, reset circuitry, an SPI™ serial port, a jumper connection for initiating ADC calibration, and an EEPROM for evaluation board identification.

The evaluation board operates from +2.5V, -2.5V, +3.3V and communicates through an SPI™ serial port.

Figure 1 illustrates the CDB5571 block diagram.


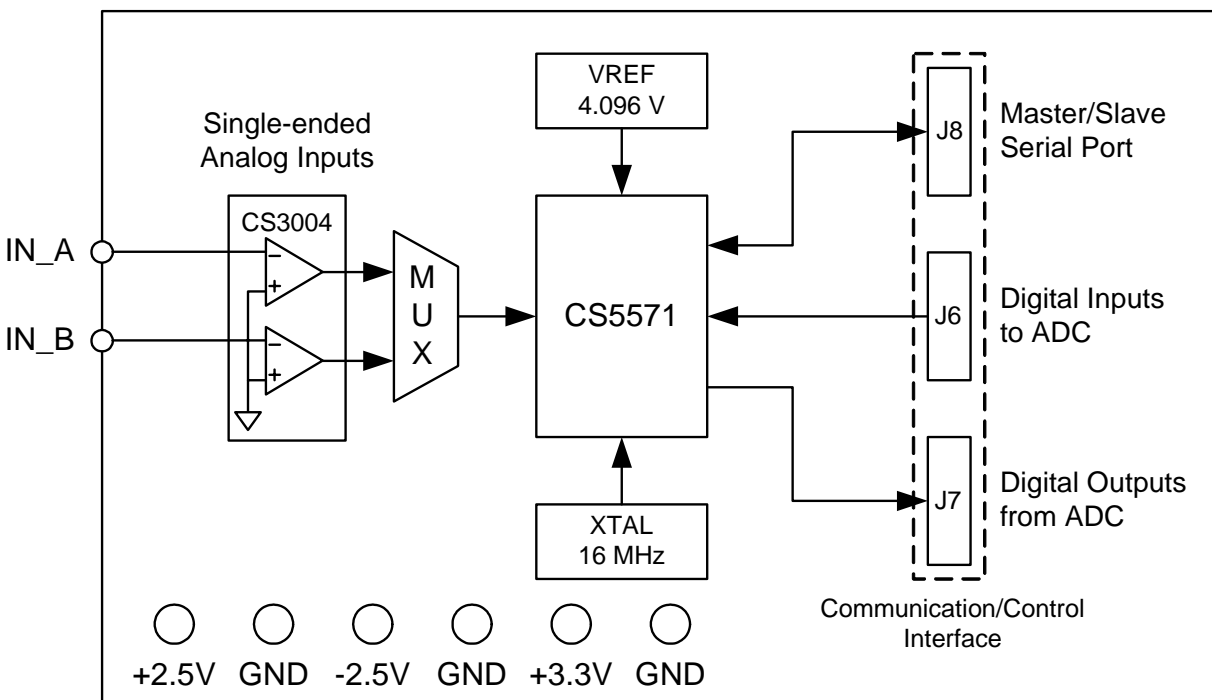


Figure 1. CDB5571 Block Diagram

## 2. QUICK START

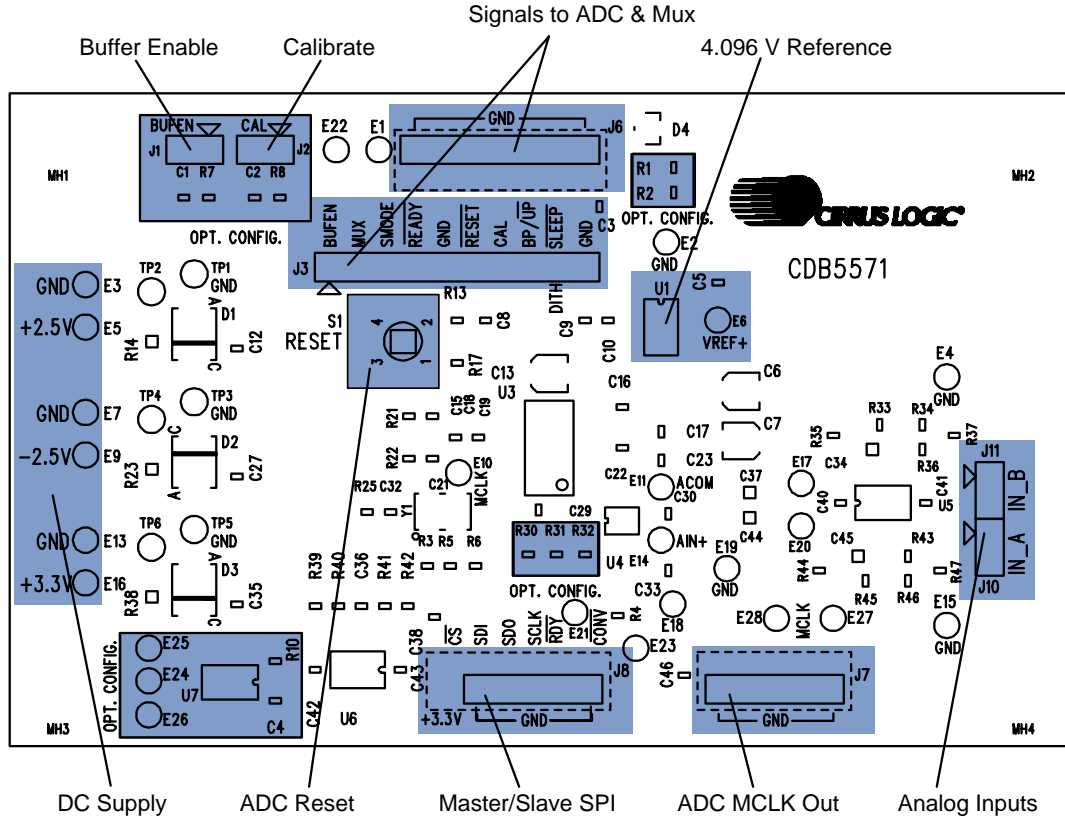

NOTE: Shaded boxes marked with "OPT. CONFIG." are not necessary for operation in an end user product.

**Figure 2. CDB5571 Board Layout**

The CDB5571 evaluation board is designed to interface with a data acquisition system. To connect and configure the CDB5571 perform the following initialization procedure:

1. Verify that the power supplies are off.
2. Connect the power supplies to the CDB5571 as shown in Table 1 on page 7.
3. Verify that the power is off to the analog input signal & control signal sources.
4. Connect the analog input signal source to the evaluation board per Table 2 on page 7. Verify from Table 4 on page 9 that the analog input channel selected is IN\_A.
5. Configure the CDB5571 by connecting the control signal sources to the evaluation board as shown in Table 3 on page 9. Apply logic-level inputs as required to override the resistor pull-ups/pull-downs.
6. Make connections to the SPI™ serial port connector as shown in Table 5 on page 9. The CS5571 ADC serial port is configured by default to operate in the SSC (Synchronous Self Clocking) mode. Refer to the CS5571 data sheet for more information on serial communication modes and signal timing.
7. Turn on the power supplies to the evaluation board.
8. Apply power to the signal source.
9. Press the Reset switch on the evaluation board.
10. The CS5571 ADC's SPI™ serial port should now be communicating data.

### 3. HARDWARE DESCRIPTION

#### 3.1 Absolute Maximum Ratings

Observe the following limits to ensure the CDB5571 component ratings are not exceeded.

- **CS5571**
  - The absolute maximum supply voltage that can be applied to the +3.3V power supply connection is +3.6V.
  - The absolute maximum power supply voltage that can be applied between pins VL and V1- is 6.1 V.
- **CS3004**
  - The absolute maximum power supply voltage that can be applied between the +2.5V and -2.5V power supply connections is +5.5V.

#### 3.2 Power Supply

Power supply connections and requirements are specified in Table 1. below.

**Table 1. Power Supply Connections**

Power Supply Requirement	Power Supply Connection	Associated Ground Return	Associated Test Points
+2.5 V DC, $\pm 5\%$ , <50 mA	E5	E3	TP2, TP1 (GND)
-2.5 V DC, $\pm 5\%$ , <50 mA	E9	E7	TP4, TP3 (GND)
+3.3 V DC, $\pm 5\%$ , <50 mA	E16	E13	TP6, TP5 (GND)

Important: It is recommended that all power supplies be isolated from utility ground to prevent the introduction of a ground loop. One ground connection may already exist through the serial port connection to utility ground. Using the Cirrus Logic CapturePlus II system simplifies making connections to the CDB5571 by providing electrical isolation between the two.

Using twisted/shielded wire will reduce electrical noise induced onto the power supply cables.

Power supplies are to be adequately regulated and sufficiently low noise to meet the application requirements.

#### 3.3 Analog Section

##### 3.3.1 Analog Input Buffers

The analog input signal connections to the input buffers are made at the IN\_A and IN\_B connectors, as specified in Table 2.

**Table 2. Analog Input Connections**

Channel	Analog Input Connection	Input Signal Voltage Range	Impedance
IN_A	J10	-2.048 V to +2.048 V	50 Ohms
IN_B	J11	-2.048 V to +2.048 V	50 Ohms

There are two analog input channels on the evaluation board. Each analog input channel consists of a low-noise amplifier configured as a unity gain non-inverting buffer. The buffers utilize a Cirrus Logic CS3004 precision, low-noise, low-voltage, dual opamp. These op-amps enable both the inputs and outputs of the analog input buffer to operate virtually rail to rail. The channel input impedance is 50 Ohms.

For detailed information on the CS3004 precision industrial op-amps, please visit the Cirrus Logic website at [www.cirrus.com](http://www.cirrus.com).

The analog inputs are designed for connections to single-ended input signals referenced to ground. The usable input voltage range is -2.048 V to +2.048 V. The theoretical input frequency range of the CS5571 is from DC to the Nyquist frequency of 50 kHz. The analog input buffer amplifiers are configured for a cut-off frequency of 16.8 kHz to band-limit noise into the ADC. Changing the cutoff frequency will change the noise bandwidth accordingly.

### 3.3.2 Multiplexer

Analog input channel selection is controlled through the multiplexer. The multiplexer is configured with a pull-down resistor on the MUX control line to enable input channel labeled "INPUT A" by default. To select channel B, apply 3.3 V to the multiplexer input control line (MUX).

Signal levels for controlling the multiplexer that selects between analog input channels A and B is shown in Table 3.

**Table 3. Analog Input Channel Selection**

Multiplexer Control Input (MUX)	Input Channel Enabled
0 V	A
3.3 V	B

During multiplexing, the maximum sample rate for each channel is half that of the ADC's maximum sample rate. Additionally, the Nyquist frequency for each channel is half of the ADC's Nyquist frequency.

### 3.3.3 ADC Reset

The CS5571 ADC makes use of an externally generated power-on reset. Therefore, after power is applied to the ADC, the reset pin must be driven low then released. Pressing the Reset button generates a reset cycle. A reset cycle can be generated at any time during ADC operation. The ADC  $\overline{\text{RST}}$  pin (active low) is held inactive through a pull-up resistor.

### 3.3.4 Voltage Reference

The voltage reference IC provided generates a 4.096 V precision reference.

### 3.3.5 ADC Reference Frequency

The reference frequency for the CS5571 ADC is provided by a 16.000 MHz oscillator.



### 3.4 Digital Section

#### 3.4.1 Hardware Configuration

The CDB5571 evaluation board hardware comes pre-configured so the only connection required between it and a data acquisition system is the serial port connection.

The hardware setup is reconfigurable through the hardware control interface connectors. Configure the evaluation board by setting the appropriate control line to the appropriate logic level.

**Table 4. Hardware Configuration Signals**

Function	Default Level	Label	Connector	Test Point
Input Channel Select	IN_A = Selected (Low)	MUX	J6, Pin 16	J3, Pin 2
Analog Input Buffers	Buffers = Enabled (High)	BUFEN	J1	J3, Pin1
Serial Port Mode	Sync. Self Clock = Enabled (High)	SMODE	J6, Pin 12	J3, Pin 3
Data Ready Flag	Data Ready When Set (Low)	$\overline{\text{RDY}}$	J8, Pin 10	J3, Pin 4
Reset	Reset = Inactive (High)	$\overline{\text{RST}}$	J6, Pin 6; S1	J3, Pin 6
Self Calibration Mode	Calibration = Inactive (Low)	CAL	J6, Pin 8; J2	J3, Pin 7
Bipolar / Unipolar Mode	Bipolar = Enabled (High)	BP / $\overline{\text{UP}}$	J6, Pin 2	J3, Pin 8
Digital Filter Dither	Dither = Enabled (High)	DITHER	J6, Pin 4	J3, Pin 9
Serial Port Communication	Chip Select = Enabled (Low)	$\overline{\text{CS}}$	J8, Pin 2	E23
Data Conversion Mode	Continuous Conversion = Active (Low)	$\overline{\text{CONV}}$	J8, Pin 12	E21

#### 3.4.2 SPI™ Serial Port Communications

The CS5571 ADC communications port features an SPI™ serial port. It can be configured for SSC mode (Master) or SEC mode (Slave) mode as shown in Table 4. Test points are provided to monitor serial communications.

Connections to the serial interface are made according to the following table.

**Table 5. Serial Interface Connections**

Function	Label	Connector	Test Point
Chip Select	$\overline{\text{CS}}$	J8, Pin 2	E23
Serial Data Input	SDI	J8, Pin 4	E24
Serial Data Output	SDO	J8, Pin 6	E25
Serial Clock	SCLK	J8, Pin 8	E26

---

## APPENDIX A. MAXIMIZING THE PERFORMANCE OF THE CS5571

### A.1 PCB Layout Considerations


- Keep the signal path short between the CS5571 ADC input capacitors C37, C44 and the ADC input pin to minimize trace inductance.
- The analog input buffer amplifiers and ADC input buffer capacitors are placed before the multiplexer. Placing the buffer amplifiers before the multiplexer allows the amplifiers driving the ADC buffer capacitors to be fully settled when sampled by the ADC. Therefore, the multiplexer must be of a low on-resistance type to prevent distortion or latency issues.
- Power supply noise is a major design consideration and the power supplies need adequate bypassing and bulk capacitance.
- When operating the ADC from +2.5 V and -2.5 V split supplies, place the power supply & buffer amplifier bypass capacitor ground connections close together.
- Keep all ground connections on each differential buffer amplifier as close to the device as possible to avoid introducing differential noise through high-impedance connections.
- Keep trace lengths short between the ADC and the voltage reference IC negative supply pins.
- Route the oscillator output away from analog circuitry.
- Use a solid ground plane in the PCB layout.
- Provide adequate separation between analog and digital signals.
- To minimize distortion within the analog signal path, consider using components with smaller voltage dependencies.
- Minimize ADC digital output edge transition current loading.


### A.2 Hardware Considerations

At a system level, use shielded cable for interconnects. Keep interconnect cable lengths as short as possible. Route analog and digital signals connecting to the PCB away from each other.

**APPENDIX B. BILL OF MATERIALS**
**BILL OF MATERIAL**
**CIRRUS LOGIC  
CDB5571\_REV\_A4.PL**

Item	Cirrus P/N	Rev	Description	Qty	Reference Designator	MFG	MFG P/N	Notes
1	001-03713-Z1	A	CAP 1000pF ±10% 50V X7R NPb 0805	2	C1 C2	KEMET	C0805C102K5RAC	
2	001-04345-Z1	A	CAP 0.1uF ±10% 50V X7R NPb 0805	27	C3 C4 C5 C9 C10 C12 C15 C16 C17 C18 C19 C21 C22 C23 C27 C29 C30 C32 C33 C35 C36 C38 C40 C41 C42 C43 C46 C6 C7 C13	KEMET	C0805C104K5RAC	
3	012-00012-Z1	A	CAP 10uF ±20% 16V ELEC NPb CASE A	3		PANASONIC	EEE1CS100SR	
4	001-03987-Z1	A	CAP 4700pF ±10% 50V X7R NPb 0805	1	C8	KEMET	C0805C472K5RAC	
5	001-05587-Z1	A	CAP 120pF ±5% 100V COG NPb 1206	2	C34 C45	KEMET	C1206C121J1GAC	
6	070-00111-Z1	A	DIODE TR 6.8V 600W NPb DO-214AA	3	D1 D2 D3	LITTELFUSE	P6SMBJ6.8A	
7	070-00010-Z1	A	DIODE SCHOTTKY BAR 30V 0.2A NPb SOT23	1	D4	PHILIPS	BAT54	
8	000-00025-Z1	A	NO POP 040 PAD 064 NPb TH	0	E1 E2 E3 E4 E5 E6 E7 E9 E10 E11 E13 E14 E15 E16 E17 E18 E19 E20 E21 E22 E23 E24 E25 E26 E27 E28	NO POP	NP-PAD-040	NO POP
9	115-00052-Z1	A	HDR 2x1 ML .1" CTR 093 GLD NPb	0	J1 J2	SAMTEC	TSW-102-26-G-S	NO POP
10	115-00217-Z1	A	HDR 10x1 FML .1" 093 GLD NPb TH	0	J3	SAMTEC	SSW-110-01-G-S	NO POP
11	115-00239-Z1	A	HDR 8x2 093BD FML .1" .331" NPb TH	1	J6	SAMTEC	SSW-108-01-G-D	
12	115-00238-Z1	A	HDR 5x2 093BD FML .1" .331" NPb TH	1	J7	SAMTEC	SSW-105-01-G-D	
13	115-00241-Z1	A	HDR 6x2 093BD FML .1" .331" NPb TH	1	J8	SAMTEC	SSW-106-01-G-D	
14	304-00012-Z1	A	SPCR STANDOFF NYL HEX750/4-40TH NPb	4	MH1 MH2 MH3 MH4	KEYSTONE	1902D	REQUIRES SCREW 4-40X1X4" PH NYLON, 300-0002-Z1
15	021-00435-Z1	A	RES 10k OHM 1/8W ±5% NPb 0805 FILM	9	R1 R2 R7 R8 R31 R32 R39 R40 R42	DALE	CRCW0805T0K0JNEA	
16	021-00363-Z1	A	RES 10 OHM 1/8W ±5% NPb 0805 FILM	4	R3 R21 R22 R25	DALE	CRCW0805T0R0JNEA	
17	020-02044-Z1	A	RES 100k OHM 1/8W ±1% NPb 0805 FILM	5	R4 R5 R6 R10 R30	DALE	CRCW0805100KFKEA	
18	020-02387-Z1	A	RES 100 OHM 1/8W ±5% NPb 0805 FILM	1	R13	DALE	CRCW0805100RJNEA	
19	020-02273-Z1	A	RES 0 OHM 1/4W 1206 FILM	3	R14 R23 R38	DALE	CRCW1206000Z0EA	
20	021-00423-Z1	A	RES 3.3k OHM 1/8W ±5% NPb 0805 FIL	1	R17	DALE	CRCW08053K300JNEA	
21	020-01848-Z1	A	RES 2k OHM 1/8W ±1% NPb 0805 FILM	4	R33 R34 R45 R46	DALE	CRCW08052K00FKEA	
22	020-00002-Z1	A	RES 49.9 OHM 1/10W ±5% NPb 0805 THN	2	R35 R44	SUSUMU	RR1220Q-49R9-D-M	
23	020-01816-Z1	A	RES 1k OHM 1/8W ±1% NPb 0805 FILM	2	R36 R43	DALE	CRCW08051K00FKEA	
24	020-01667-Z1	A	RES 49.9 OHM 1/8W ±1% NPb 0805 FILM	2	R37 R47	DALE	CRCW080549R9FKEA	
25	021-01430-Z1	A	RES 33k OHM 1/8W ±5% NPb 0805 FILM	1	R41	DALE	CRCW080533K0JNEA	
26	120-00057-Z1	A	SWT SPST 130G 0/1 7mm TACT ESD NPb	1	S1	ITT INDUSTRIES	PTS645TL70	INSTALL AFTER WASH PROCESS
27	110-00045-Z1	A	CON TEST PT .1" CTR TIN PLAT NPb BLK	3	TP1 TP3 TP5	KEYSTONE	5001	
28	110-00024-Z1	A	CON TEST PT .1" TIN PLT RED NPb TH	2	TP2 TP6	KEYSTONE	5000	
29	110-00025-Z1	A	CON TEST PT .1" TIN PLATE WHT NPb	1	TP4	KEYSTONE	5002	
30	060-00351-Z1	A	IC LNR PREC VREF 4.096V/out NPb SO8	1	U1	MAXIM	MAX6126AASA41+	
31	065-00238-Z3	B0	IC CRUS ADC 100kSps 16b NPb SSOP24	1	U3	CIRRUS LOGIC	CS5571-JSZB0	ECO521, ECO542
32	060-00352-Z1	A	IC LNR ANA SW 4OHM SPDT NPb MSOP10	1	U4	MAXIM	MAX4635EUB+	
33	065-00219-Z1	A0	IC CRUS PREC DL LO-V AMP NPb SOIC8	1	U5	CIRRUS LOGIC	CS3004-FSZ/A0	
34	060-00386-Z1	A	IC LNR DIFF COMP HS 5.25V NPb SOIC8	1	U6	TEXAS INSTRUMENTS	TL712CD	
35	062-00064-Z1	A	IC PGM SPI EEPROM 8Kx8 2MHz NPb SO8	1	U7	MICROCHIP	25LC640-I/SN	
36	102-00097-Z1	A	OSC 16MHz 50ppm 3.3V NPb SMD 3x5	1	Y1	ABRACON	ASFL1-16.000MHZ-EC-T	
37	603-00284-Z1	A	ASSY DWG CDB5571-1-Z NPb	REF		CIRRUS LOGIC	603-00284-Z1	
38	240-00284-Z1	A	PCB CDB5571-1-Z NPb	1		CIRRUS LOGIC	240-00284-Z1	
39	600-00284-Z1	A4	SCHEM CDB5571-Z NPb	REF		CIRRUS LOGIC	600-00284-Z1	ECO521, ECO542
40	300-00002-Z1	A	SCREW 4-40X1/4" PH NYLON NPb	4	XMH1 XMH2 XMH3 XMH4	BUILDING FASTENERS	NY PMS 440 0025 PH	
41	001-06472-Z1	A	CAP 4700pF ±5% 50V COG NPb 1206	2	C37 C44	KEMET	C1206C472J5GAC	
42	115-00052-Z1	A	HDR 2x1 ML .1" CTR 093 GLD NPb	2	J10 J11	SAMTEC	TSW-102-26-G-S	

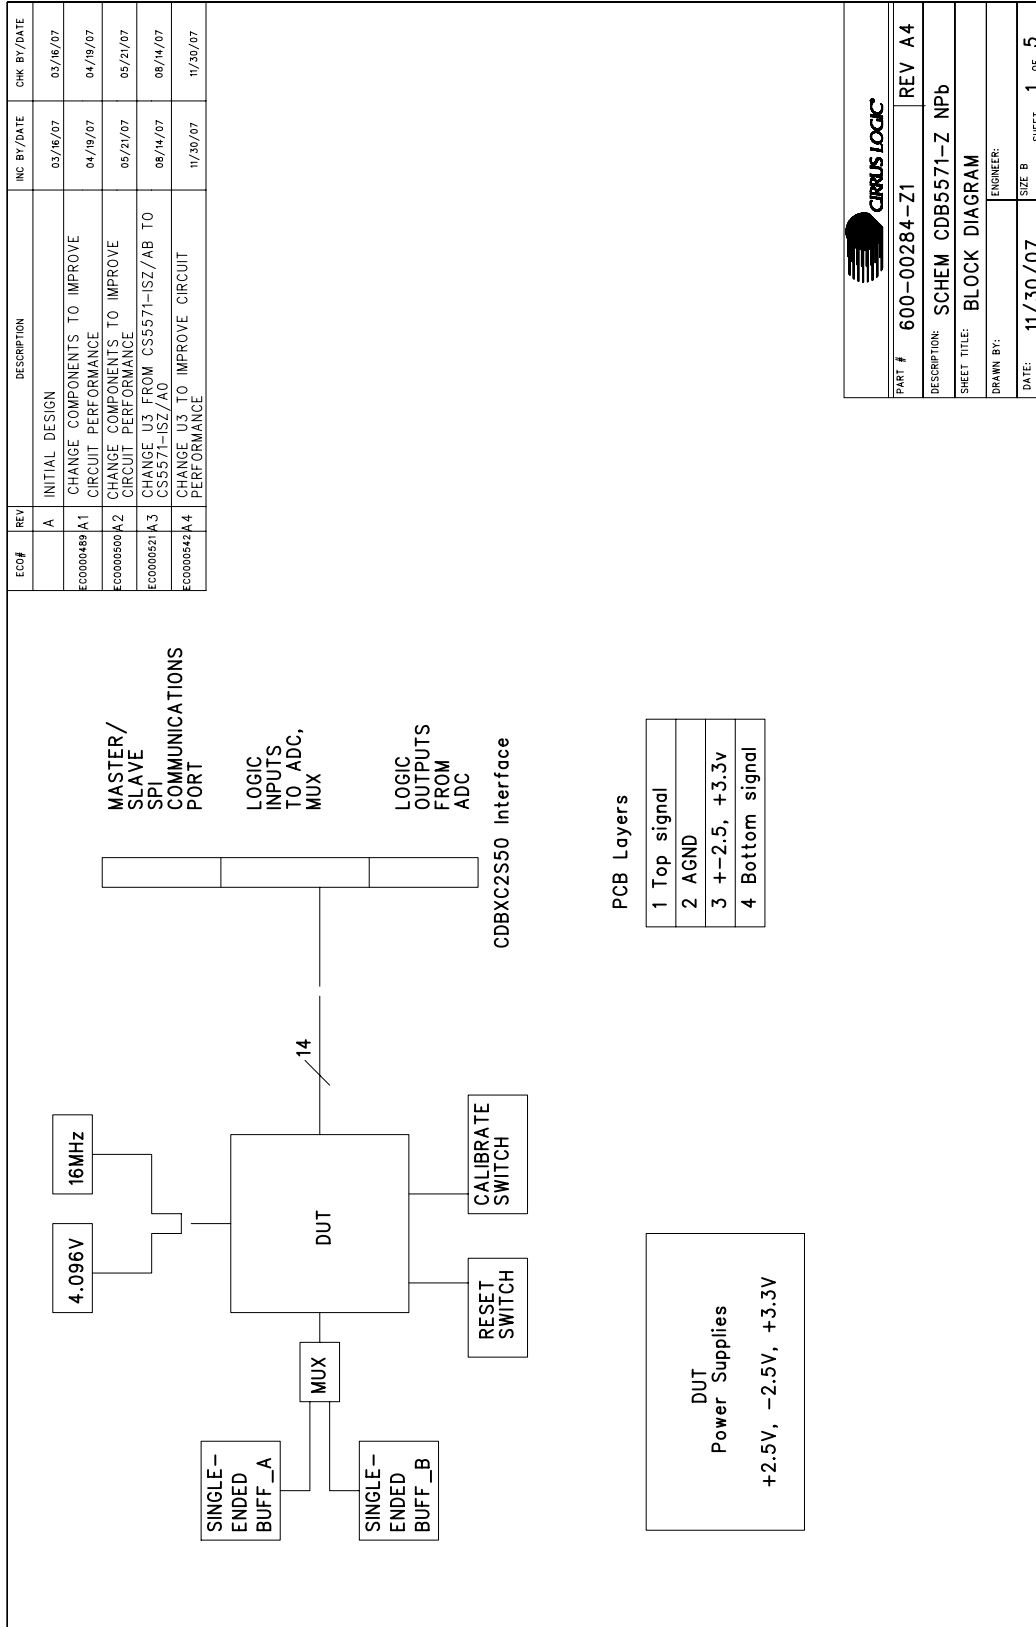**APPENDIX C. SCHEMATICS**

**Figure 3. Schematic - Block Diagram**


**Figure 4. Schematic - Power Supplies**




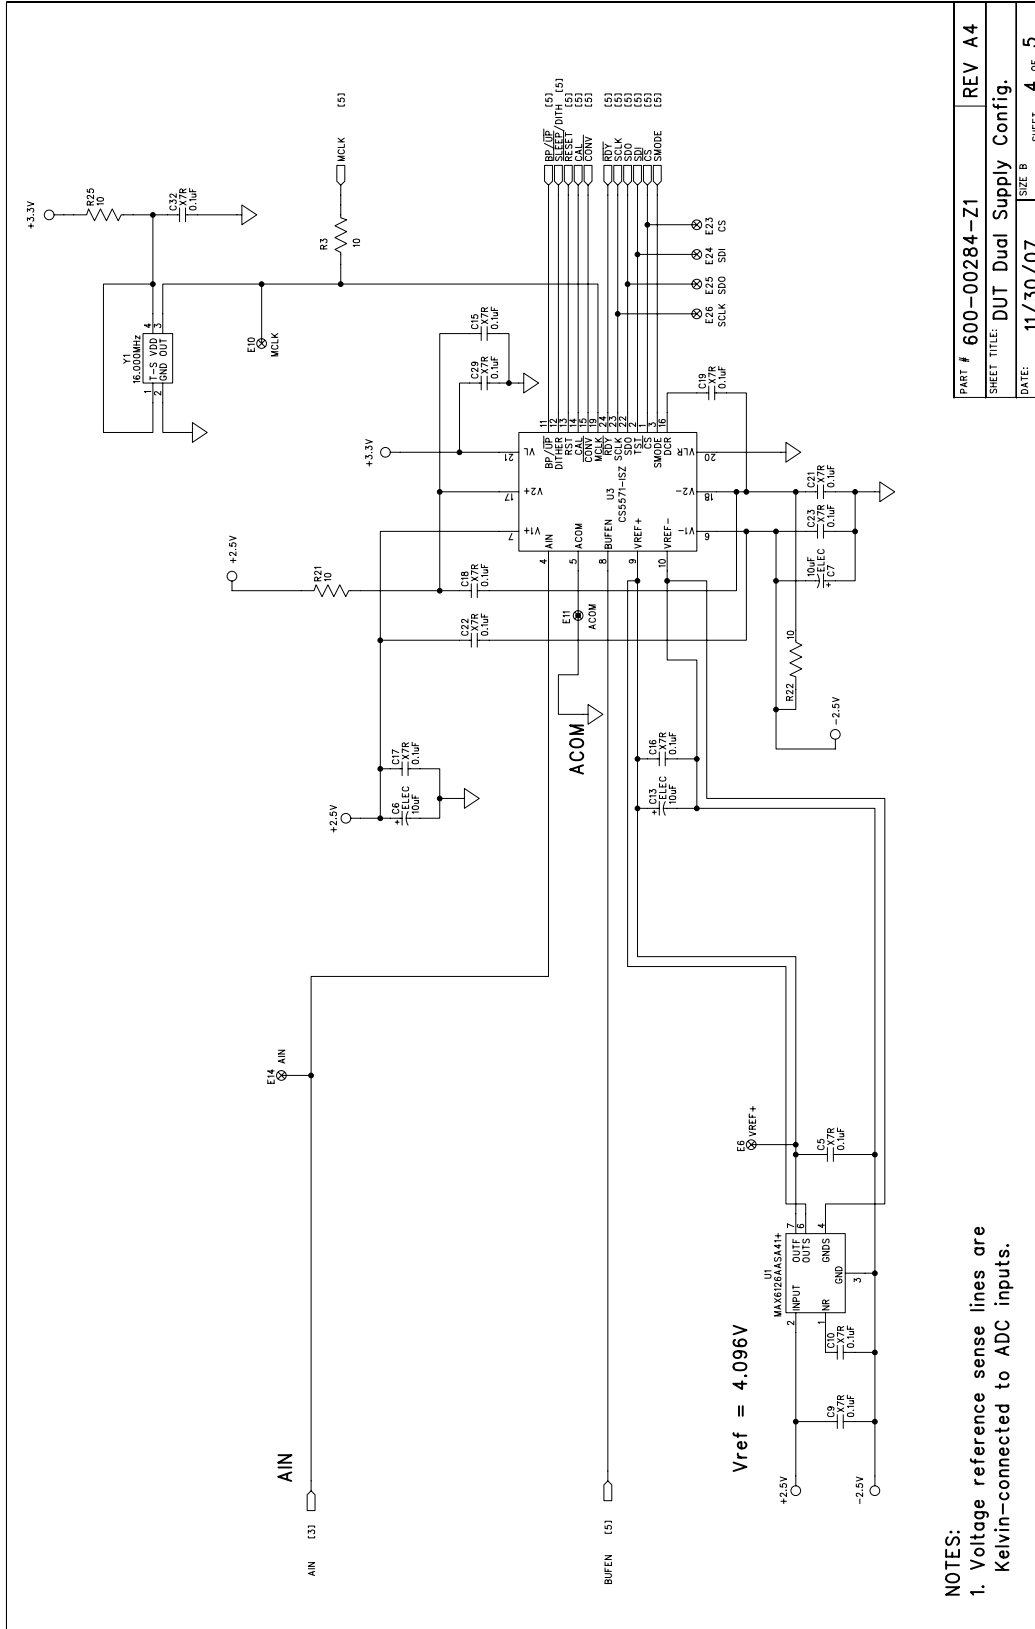


Figure 6. Schematic - CS5571




PART #	600-00284-Z1	REV	A4
SHEET TITLE:	Support Components		
DATE:	11/30/07	SHEET	5 OF 5

Figure 7. Schematic - Configuration & Misc.

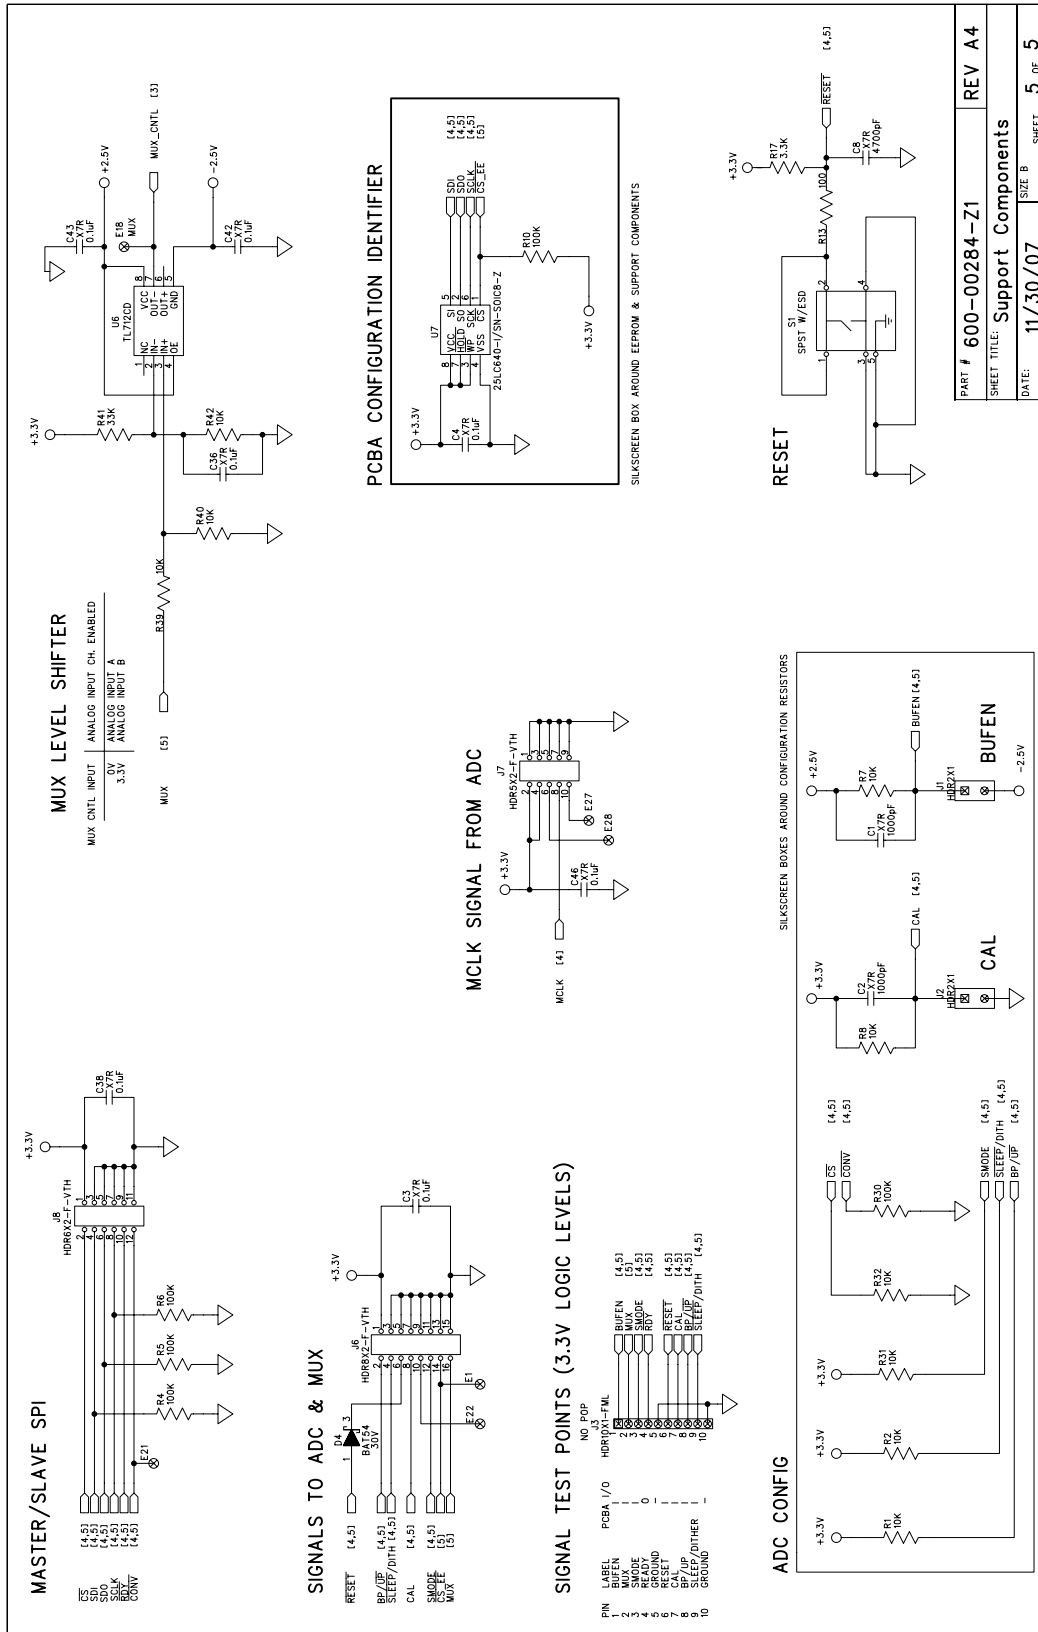






CIRRUS LOGIC 240-00284-Z1 REV A

SOLDERMASK TOP

Figure 9. Top Solder Mask






CIRRUS LOGIC 240-00284-Z1 REV A

TOP SIDE

Figure 10. Top Routing






CIRRUS LOGIC 240-00284-Z1 REV A

INNER LAYER 2 (GND)

Figure 11. Ground Plane






CIRRUS LOGIC 240-00284-Z1 REV A

INNER LAYER 3 (PWR)


Figure 12. Power Plane



CIRRUS LOGIC 240-00284-Z1 REV A

SOLDERMASK BOTTOM  
Figure 13. Bottom Solder Mask






SILKSCREEN BOTTOM

CIRRUS LOGIC S40-00584-S1 REV A

Figure 14. Bottom Silkscreen




CIRRUS LOGIC 240-00284-Z1 REV A

PASTE MASK TOP

Figure 15. Top Solder Paste Mask







CIRRUS LOGIC 240-00284-Z1 REV A

BOTTOM SIDE

Figure 16. Bottom Routing



---

**REVISION HISTORY**

<b>Revision</b>	<b>Date</b>	<b>Changes</b>
DB1	APR 2007	Initial Release.
DB2	AUG 2007	Added 3.3.2 Multiplexer section.
DB3	DEC 2007	Updated schematic to reflect new silicon revision.